

## **EXAMPLE OF LABELS MULTIGEN PLUS KNEE SYSTEM**

Label of the first code of each kind of device for Multigen Plus Knee System is following reported. For each label, all the information which changes in the other labels of the same device is showed.

The labels are reported as follows:

Section 1	Example of labels for Femoral Components
Section 2	Example of labels for Tibial Plates
Section 3	Example of labels for Tibial Liners (UHMWPE)
Section 4	Example of labels for Multigen Plus – CCK
Section 5	Example of labels for Multigen Plus – H
Section 6	Example of labels for Augments (Ti6Al4V)
Section 7	Example of labels for Stems (Ti6Al4V) and Modules (Ti6Al4V)
Section 8	Example of labels for Patellar Prosthesis (UHMWPE)

## **STERILIZATION – DATA ON THE LABELS**

The information about the sterilization method for the device is reported on the labels. The external cardboard box (first label in each of the following pages) indicates only the possible sterilization methods:



- **STERILE R:** sterilization by **irradiation** (Beta rays or Gamma rays according to the applicable sterilization method).



- **STERILE EO:** sterilization by **ethylene oxide**.

Always refer to device labels for information about the sterilization method.


For the information on applicable sterilization method for each device refer to Design Dossier.

**SECTION 1 – EXAMPLE OF LABELS FOR FEMORAL COMPONENTS**

**Data Legend**

(the information which changes in the other labels of the same device is squared and showed in the table below).

- **Cemented Femoral Components**

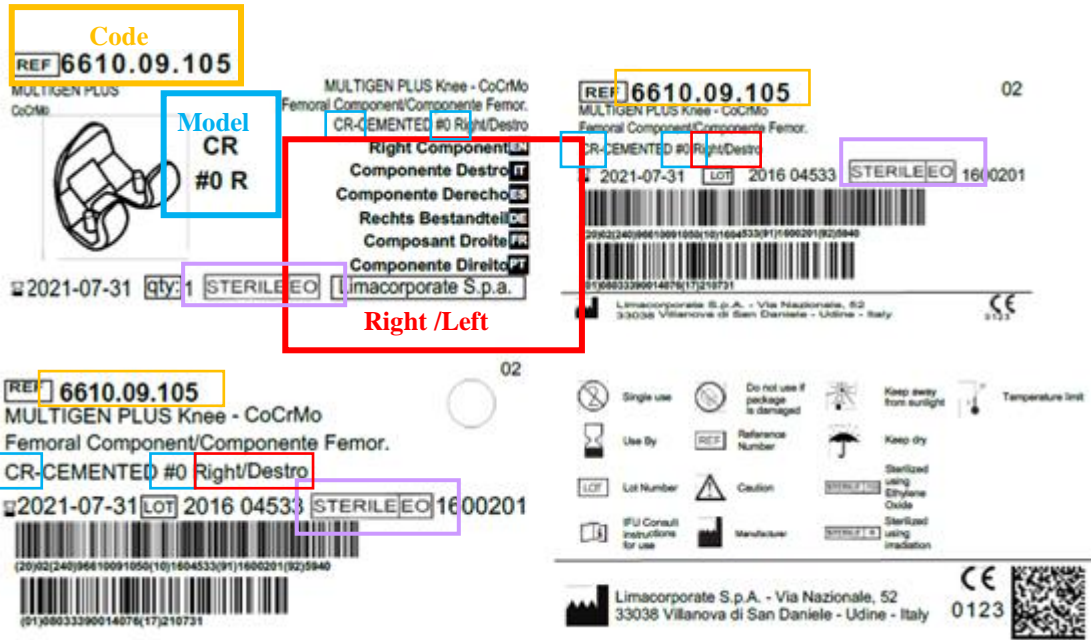

Code	Model	Right/Left	Sterilization method
6610.09.105	CR #0 R	Right	EtO/Gamma
6610.09.110	CR #1 R	Right	EtO/Gamma
6610.09.120	CR #2 R	Right	EtO/Gamma
6610.09.130	CR #3 R	Right	EtO/Gamma
6610.09.140	CR #4 R	Right	EtO/Gamma
6610.09.150	CR #5 R	Right	EtO/Gamma
6610.09.205	CR #0 L	Left	EtO/Gamma
6610.09.210	CR #1 L	Left	EtO/Gamma
6610.09.220	CR #2 L	Left	EtO/Gamma
6610.09.230	CR #3 L	Left	EtO/Gamma
6610.09.240	CR #4 L	Left	EtO/Gamma
6610.09.250	CR #5 L	Left	EtO/Gamma
6612.09.105	PS #0 R	Right	EtO/Gamma
6612.09.110	PS #1 R	Right	EtO/Gamma
6612.09.120	PS #2 R	Right	EtO/Gamma
6612.09.130	PS #3 R	Right	EtO/Gamma

Code	Model	Right/Left	Sterilization method
6612.09.140	PS #4 R	Right	EtO/Gamma
6612.09.150	PS #5 R	Right	EtO/Gamma
6612.09.205	PS #0 L	Left	EtO/Gamma
6612.09.210	PS #1 L	Left	EtO/Gamma
6612.09.220	PS #2 L	Left	EtO/Gamma
6612.09.230	PS #3 L	Left	EtO/Gamma
6612.09.240	PS #4 L	Left	EtO/Gamma
6612.09.250	PS #5 L	Left	EtO/Gamma

• **Uncemented Femoral Components**

**Code**  
REF 6610.10.105  
MULTIGEN PLUS  
CoCrMo+PorTi


**Model**  
CR  
#0 R

2024-07-31 Qty 1 STERILE EO Limacorporate S.p.a.

MULTIGEN PLUS Knee - CoCrMo+PorTi  
Femoral Component  
CR - UNCEMENTED #0 - Right

Right Component EN  
Componente Destro IT  
Componente Derecho ES  
Rechts Bestandteil DE  
Composant Droite FR  
Componente Direito PT

**Right / Left**



REF 6610.10.105 02  
MULTIGEN PLUS Knee - CoCrMo+PorTi  
Femoral Component  
CR - UNCEMENTED #0 - Right

2024-07-31 LOT 2019 01 001 STERILE EO 1900002

0200224010010101050101900000191190030222113

011003336001425017240731  
Limacorporate S.p.A. - Via Nazionale, 52  
33036 Villanova di San Daniele - Udine - Italy

CE 0123

REF 6610.10.105 02  
MULTIGEN PLUS Knee - CoCrMo+PorTi  
Femoral Component  
CR - UNCEMENTED #0 - Right

2024-07-31 LOT 2019 00001 STERILE EO 1900002

0200224010010101050101900000191190030222113

011003336001425017240731

Single use Do not use if package is damaged Keep away from sunlight Temperature limit

Use by REF Reference Number Keep dry MIT Conditional

LOT Lot Number Caution Sterilized using Ethylene Oxide

IFU Consult instructions for use Manufacture Sterilized using irradiation

Limacorporate S.p.A. - Via Nazionale, 52  
33036 Villanova di San Daniele - Udine - Italy

CE 0123


**Code**  
REF 6612.10.105  
MULTIGEN PLUS  
CoCrMo+PorTi

**Model**  
PS  
#0 R

2024-07-31 Qty 1 STERILE EO Limacorporate S.p.a.


MULTIGEN PLUS Knee - CoCrMo+PorTi  
Femoral Component  
PS-UNCEMENTED #0 Right

Right Component EN  
Componente Destro IT  
Componente Derecho ES  
Rechts Bestandteil DE



REF 6612.10.105 03  
MULTIGEN PLUS Knee - CoCrMo+PorTi  
Femoral Component  
PS-UNCEMENTED #0 Right

2024-07-31 LOT 2019 00001 STERILE EO 1900002

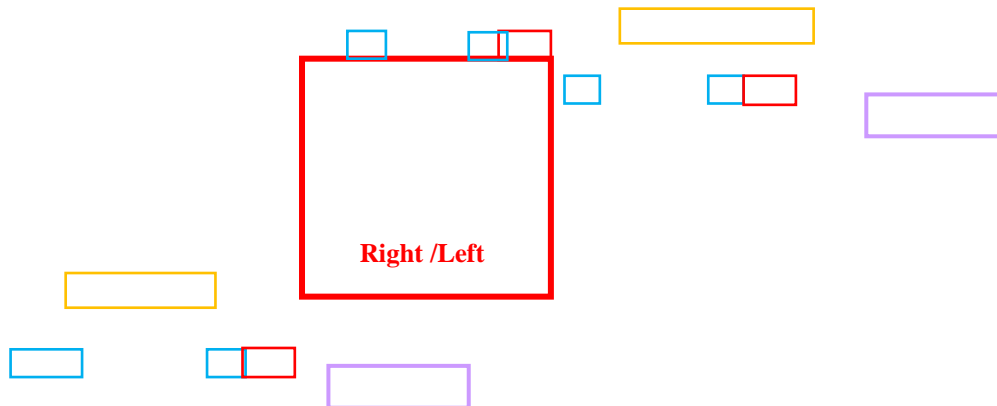


Code	Model	Right/Left	Sterilization method
6610.10.105	CR #0 R	Right	EtO/Gamma
6610.10.110	CR #1 R	Right	EtO/Gamma
6610.10.120	CR #2 R	Right	EtO/Gamma
6610.10.130	CR #3 R	Right	EtO/Gamma
6610.10.140	CR #4 R	Right	EtO/Gamma
6610.10.150	CR #5 R	Right	EtO/Gamma
6610.10.205	CR #0 L	Left	EtO/Gamma
6610.10.210	CR #1 L	Left	EtO/Gamma
6610.10.220	CR #2 L	Left	EtO/Gamma
6610.10.230	CR #3 L	Left	EtO/Gamma
6610.10.240	CR #4 L	Left	EtO/Gamma
6610.10.250	CR #5 L	Left	EtO/Gamma
6612.10.105	PS #0 R	Right	EtO/Gamma
6612.10.110	PS #1 R	Right	EtO/Gamma
6612.10.120	PS #2 R	Right	EtO/Gamma
6612.10.130	PS #3 R	Right	EtO/Gamma
6612.10.140	PS #4 R	Right	EtO/Gamma
6612.10.150	PS #5 R	Right	EtO/Gamma
6612.10.205	PS #0 L	Left	EtO/Gamma
6612.10.210	PS #1 L	Left	EtO/Gamma
6612.10.220	PS #2 L	Left	EtO/Gamma
6612.10.230	PS #3 L	Left	EtO/Gamma
6612.10.240	PS #4 L	Left	EtO/Gamma
6612.10.250	PS #5 L	Left	EtO/Gamma

**SECTION 2 – EXAMPLE OF LABELS FOR TIBIAL PLATES**

**Data Legend**


(the information which changes in the other labels of the same device is squared and showed in the table below).

• **Cemented Tibial Plates**

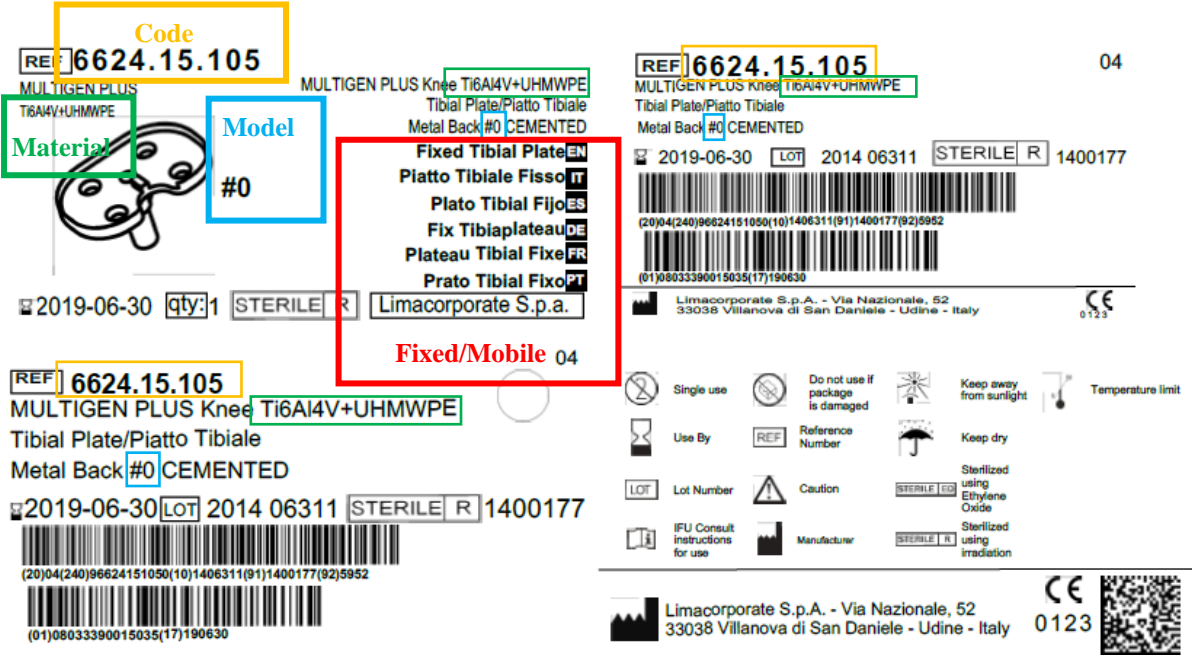

Code	Model	Material	Fixed/Mobile
6624.15.105	#0	Ti6Al4V+UHMWPE	Fixed
6624.15.110	#1	Ti6Al4V+UHMWPE	Fixed
6624.15.120	#2	Ti6Al4V+UHMWPE	Fixed
6624.15.130	#3	Ti6Al4V+UHMWPE	Fixed
6624.15.140	#4	Ti6Al4V+UHMWPE	Fixed
6624.15.150	#5	Ti6Al4V+UHMWPE	Fixed
6623.09.005	#0	CoCrMo	Mobile
6623.09.010	#1	CoCrMo	Mobile
6623.09.020	#2	CoCrMo	Mobile
6623.09.030	#3	CoCrMo	Mobile
6623.09.040	#4	CoCrMo	Mobile
6623.09.050	#5	CoCrMo	Mobile

• **Uncemented Tibial Plates**



REF 6624.21.105 MULTIGEN PLUS Knee - Ti6Al4V+PoroTi Tibial Plate 04

MULTIGEN PLUS Ti6Al4V+PoroTi **Material** #0

Fixed Tibial Plate EN  
Piatto Tibiale Fisso IT  
Plato Tibial Fijo ES  
Fix Tibiplateau DE  
Plateau Tibial Fixe FR  
Prato Tibial Fixo PT

Metal Back #0 UNCEMENTED

2024-07-31 Qty 1 STERILE EO Limacorporate S.p.a. **Fixed/Mobile**

REF 6624.21.105 MULTIGEN PLUS Knee - Ti6Al4V+PoroTi Tibial Plate 04

Metal Back #0 UNCEMENTED

2024-07-31 LOT 2019 00001 STERILE EO 1900002

01J08033390015156(17)240731  
Limacorporate S.p.A. - Via Nazionale, 52  
33038 Villanova di San Daniele - Udine - Italy

CE 0123

REF 6624.21.105 04

MULTIGEN PLUS Knee - Ti6Al4V+PoroTi Tibial Plate

Metal Back #0 UNCEMENTED

2024-07-31 LOT 2019 00001 STERILE EO 1900002

01J08033390015156(17)240731

Single use Do not use if package is damaged Keep away from sunlight Temperature limit

Use by REF Reference Number Keep dry MR Conditional

LOT Lot Number Caution STERILE EO Sterilized using Ethylene Oxide

IFU Consult instructions for use Manufacturer STERILE EO Sterilized using irradiation

Limacorporate S.p.A. - Via Nazionale, 52  
33038 Villanova di San Daniele - Udine - Italy

CE 0123

REF 6623.10.005 MULTIGEN PLUS Knee - CoCrMo+PoroTi Tibial Plate 07

MULTIGEN PLUS CoCrMo+PoroTi **Material** #0 **Model**

Mobile Tibial Plate EN  
Piatto Tib. Mobile IT  
Plato Tibial Movil ES  
Mobil Tibiplateau DE  
Plateau Tibial Mobile FR  
Prato Tibial Movel PT

#0 - Mobile Uncemented

2024-07-31 Qty 1 STERILE EO Limacorporate S.p.a. **Fixed/Mobile**

REF 6623.10.005 MULTIGEN PLUS Knee - CoCrMo+PoroTi Tibial Plate 07

#0 - Mobile Uncemented

2024-07-31 LOT 2019 00001 STERILE EO 1900002

01J08033390014915(17)240731

REF 6623.10.005 07

MULTIGEN PLUS Knee - CoCrMo+PoroTi Tibial Plate

#0 - Mobile Uncemented

2024-07-31 LOT 2019 00001 STERILE EO 1900002

01J08033390014915(17)240731  
Limacorporate S.p.A. - Via Nazionale, 52  
33038 Villanova di San Daniele - Udine - Italy

CE 0123

Single use Do not use if package is damaged Keep away from sunlight Temperature limit

Use by REF Reference Number Keep dry MR Conditional

LOT Lot Number Caution STERILE EO Sterilized using Ethylene Oxide

IFU Consult instructions for use Manufacturer STERILE EO Sterilized using irradiation

Limacorporate S.p.A. - Via Nazionale, 52  
33038 Villanova di San Daniele - Udine - Italy

CE 0123


Code	Model	Material	Fixed/Mobile
6624.21.105	#0	Ti6Al4V+PoroTi	Fixed
6624.21.110	#1	Ti6Al4V+PoroTi	Fixed
6624.21.120	#2	Ti6Al4V+PoroTi	Fixed
6624.21.130	#3	Ti6Al4V+PoroTi	Fixed
6624.21.140	#4	Ti6Al4V+PoroTi	Fixed

6624.21.150	#5	Ti6Al4V+PoroTi	Fixed
6623.10.005	#0	CoCrMo + PoroTi	Mobile
6623.10.010	#1	CoCrMo + PoroTi	Mobile
6623.10.020	#2	CoCrMo + PoroTi	Mobile
6623.10.030	#3	CoCrMo + PoroTi	Mobile
6623.10.040	#4	CoCrMo + PoroTi	Mobile
6623.10.050	#5	CoCrMo + PoroTi	Mobile

**SECTION 3 – EXAMPLE OF LABELS FOR TIBIAL LINER (UHMWPE)**

**Data Legend**

(the information which changes in the other labels of the same device is squared and showed in the table below).

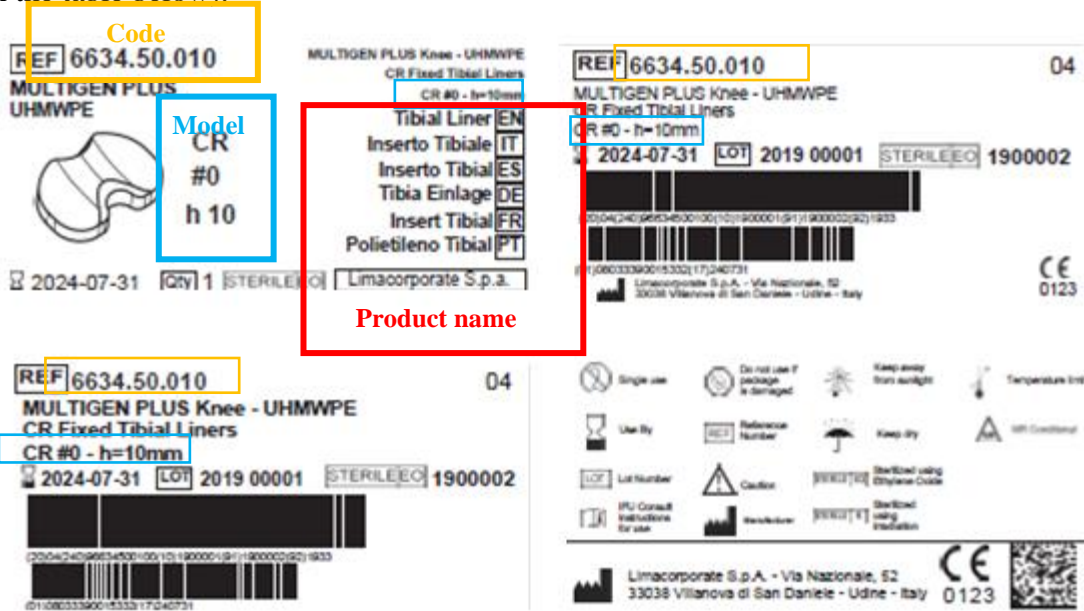


The image shows three examples of product labels for Tibial Liner (UHMWPE) with highlighted data points:

- Code:** REF 6634.50.010 (highlighted in yellow)
- Model:** CR #0 h 10 (highlighted in blue)
- Product name:** Tibial Liner (highlighted in red)

The labels include the following information:

- Product Name: MULTIGEN PLUS Knee - UHMWPE CR Fixed Tibial Liners
- Model: CR #0 - h=10mm
- Lot Number: 2024-07-31
- Lot Number: 2019 00001
- Sterility: STERILE
- Quantity: Qty 1
- Manufacturer: Lima corporate S.p.a.
- CE Marking: CE 0123
- Barcode: (02062409205450010010190000101190000202) 933
- Barcode: (01100033390015332117240731)
- Instructions: Single use, Do not use if package is damaged, Keep away from sunlight, Temperature limit, Use by, Reference Number, Keep dry, Lot Number, Caution, Sterilized using Ethylene Oxide, IPU Consult instructions for use, Sterilized using irradiation.
- Manufacturer Address: Lima corporate S.p.A. - Via Nazionale, 52 33038 Villanova di San Daniele - Udine - Italy

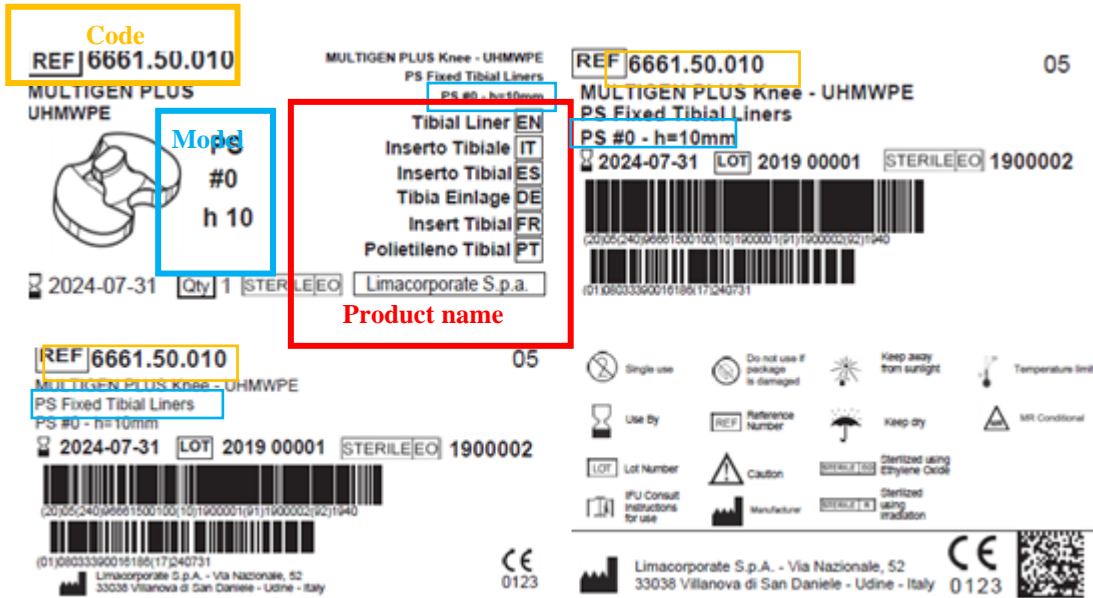

**Code**  
REF|6661.50.010

**Model**  
#0  
h 10

**Product name**

MULTIGEN PLUS Knee - UHMWPE  
PS Fixed Tibial Liners  
PS #0 - h=10mm

Tibial Liner EN  
Inserto Tibiale IT  
Inserto Tibial ES  
Tibia Einlage DE  
Insert Tibial FR  
Polietileno Tibial PT

REF|6661.50.010 05  
MULTIGEN PLUS Knee - UHMWPE  
PS Fixed Tibial Liners  
PS #0 - h=10mm  
2024-07-31 LOT 2019 00001 STERILE/EO 1900002

Single use Do not use if package is damaged Keep away from sunlight Temperature limit  
Use by REF Reference Number Keep dry MR Conditional  
LOT Lot Number Caution Sterilized using Ethylene Oxide  
IFU Consult instructions for use Manufacture Sterilized using irradiation

CE 0123 Limacorporate S.p.A. - Via Nazionale, 52 33038 Villanova di San Daniele - Udine - Italy

Code	Model	Product name
6634.50.010	CR #0 h. 10 mm	CR fixed Tibial Liner
6634.50.020	CR #0 h. 12 mm	CR fixed Tibial Liner
6634.50.030	CR #0 h. 14 mm	CR fixed Tibial Liner
6634.50.040	CR #0 h. 17 mm	CR fixed Tibial Liner
6634.50.050	CR #0 h. 20 mm	CR fixed Tibial Liner
6635.50.010	CR #1 h. 10 mm	CR fixed Tibial Liner
6635.50.020	CR #1 h. 12 mm	CR fixed Tibial Liner
6635.50.030	CR #1 h. 14 mm	CR fixed Tibial Liner
6635.50.040	CR #1 h. 17 mm	CR fixed Tibial Liner
6635.50.050	CR #1 h. 20 mm	CR fixed Tibial Liner
6637.50.010	CR #2 h. 10 mm	CR fixed Tibial Liner
6637.50.020	CR #2 h. 12 mm	CR fixed Tibial Liner
6637.50.030	CR #2 h. 14 mm	CR fixed Tibial Liner
6637.50.040	CR #2 h. 17 mm	CR fixed Tibial Liner
6637.50.050	CR #2 h. 20 mm	CR fixed Tibial Liner
6639.50.010	CR #3 h. 10 mm	CR fixed Tibial Liner
6639.50.020	CR #3 h. 12 mm	CR fixed Tibial Liner
6639.50.030	CR #3 h. 14 mm	CR fixed Tibial Liner
6639.50.040	CR #3 h. 17 mm	CR fixed Tibial Liner
6639.50.050	CR #3 h. 20 mm	CR fixed Tibial Liner
6641.50.010	CR #4 h. 10 mm	CR fixed Tibial Liner
6641.50.020	CR #4 h. 12 mm	CR fixed Tibial Liner
6641.50.030	CR #4 h. 14 mm	CR fixed Tibial Liner
6641.50.040	CR #4 h. 17 mm	CR fixed Tibial Liner
6641.50.050	CR #4 h. 20 mm	CR fixed Tibial Liner



6643.50.010	CR #5 h. 10 mm	CR fixed Tibial Liner
6643.50.020	CR #5 h. 12 mm	CR fixed Tibial Liner
6643.50.030	CR #5 h. 14 mm	CR fixed Tibial Liner
6643.50.040	CR #5 h. 17 mm	CR fixed Tibial Liner
6643.50.050	CR #5 h. 20 mm	CR fixed Tibial Liner
6668.50.010	UC #0 h. 10 mm	UC fixed tibial liner
6668.50.012	UC #0 h. 12 mm	UC fixed tibial liner
6668.50.014	UC #0 h. 14 mm	UC fixed tibial liner
6668.50.017	UC #0 h. 17 mm	UC fixed tibial liner
6668.50.020	UC #0 h. 20 mm	UC fixed tibial liner
6668.50.110	UC #1 h. 10 mm	UC fixed tibial liner
6668.50.112	UC #1 h. 12 mm	UC fixed tibial liner
6668.50.114	UC #1 h. 14 mm	UC fixed tibial liner
6668.50.117	UC #1 h. 17 mm	UC fixed tibial liner
6668.50.120	UC #1 h. 20 mm	UC fixed tibial liner
6668.50.210	UC #2 h. 10 mm	UC fixed tibial liner
6668.50.212	UC #2 h. 12 mm	UC fixed tibial liner
6668.50.214	UC #2 h. 14 mm	UC fixed tibial liner
6668.50.217	UC #2 h. 17 mm	UC fixed tibial liner
6668.50.220	UC #2 h. 20 mm	UC fixed tibial liner
6668.50.310	UC #3 h. 10 mm	UC fixed tibial liner
6668.50.312	UC #3 h. 12 mm	UC fixed tibial liner
6668.50.314	UC #3 h. 14 mm	UC fixed tibial liner
6668.50.317	UC #3 h. 17 mm	UC fixed tibial liner
6668.50.320	UC #3 h. 20 mm	UC fixed tibial liner
6668.50.410	UC #4 h. 10 mm	UC fixed tibial liner
6668.50.412	UC #4 h. 12 mm	UC fixed tibial liner
6668.50.414	UC #4 h. 14 mm	UC fixed tibial liner
6668.50.417	UC #4 h. 17 mm	UC fixed tibial liner
6668.50.420	UC #4 h. 20 mm	UC fixed tibial liner
6668.50.510	UC #5 h. 10 mm	UC fixed tibial liner
6668.50.512	UC #5 h. 12 mm	UC fixed tibial liner
6668.50.514	UC #5 h. 14 mm	UC fixed tibial liner
6668.50.517	UC #5 h. 17 mm	UC fixed tibial liner
6668.50.520	UC #5 h. 20 mm	UC fixed tibial liner
6661.50.010	PS #0 h. 10 mm	PS fixed Tibial liner
6661.50.012	PS #0 h. 12 mm	PS fixed Tibial liner
6661.50.014	PS #0 h. 14 mm	PS fixed Tibial liner
6661.50.017	PS #0 h. 17 mm	PS fixed Tibial liner
6661.50.020	PS #0 h. 20 mm	PS fixed Tibial liner
6661.50.110	PS #1 h. 10 mm	PS fixed Tibial liner
6661.50.112	PS #1 h. 12 mm	PS fixed Tibial liner
6661.50.114	PS #1h. 14 mm	PS fixed Tibial liner

6661.50.117	PS #1 h. 17 mm	PS fixed Tibial liner
6661.50.120	PS #1 h. 20 mm	PS fixed Tibial liner
6661.50.210	PS #2 h. 10 mm	PS fixed Tibial liner
6661.50.212	PS #2 h. 12 mm	PS fixed Tibial liner
6661.50.214	PS #2 h. 14 mm	PS fixed Tibial liner
6661.50.217	PS #2 h. 17 mm	PS fixed Tibial liner
6661.50.220	PS #2 h. 20 mm	PS fixed Tibial liner
6661.50.310	PS #3 h. 10 mm	PS fixed Tibial liner
6661.50.312	PS #3 h. 12 mm	PS fixed Tibial liner
6661.50.314	PS #3 h. 14 mm	PS fixed Tibial liner
6661.50.317	PS #3 h. 17 mm	PS fixed Tibial liner
6661.50.320	PS #3 h. 20 mm	PS fixed Tibial liner
6661.50.410	PS #4 h. 10 mm	PS fixed Tibial liner
6661.50.412	PS #4 h. 12 mm	PS fixed Tibial liner
6661.50.414	PS #4 h. 14 mm	PS fixed Tibial liner
6661.50.417	PS #4 h. 17 mm	PS fixed Tibial liner
6661.50.420	PS #4 h. 20 mm	PS fixed Tibial liner
6661.50.510	PS #5 h. 10 mm	PS fixed Tibial liner
6661.50.512	PS #5 h. 12 mm	PS fixed Tibial liner
6661.50.514	PS #5 h. 14 mm	PS fixed Tibial liner
6661.50.517	PS #5 h. 17 mm	PS fixed Tibial liner
6661.50.520	PS #5 h. 20 mm	PS fixed Tibial liner
6663.50.010	CR #0 h. 10 mm	CR Mobile Tibial liner
6663.50.012	CR #0 h. 12 mm	CR Mobile Tibial liner
6663.50.014	CR #0 h. 14 mm	CR Mobile Tibial liner
6663.50.017	CR #0 h. 17 mm	CR Mobile Tibial liner
6663.50.020	CR #0 h. 20 mm	CR Mobile Tibial liner
6663.50.110	CR #1 h. 10 mm	CR Mobile Tibial liner
6663.50.112	CR #1 h. 12 mm	CR Mobile Tibial liner
6663.50.114	CR #1h. 14 mm	CR Mobile Tibial liner
6663.50.117	CR #1 h. 17 mm	CR Mobile Tibial liner
6663.50.120	CR #1 h. 20 mm	CR Mobile Tibial liner
6663.50.210	CR #2 h. 10 mm	CR Mobile Tibial liner
6663.50.212	CR #2 h. 12 mm	CR Mobile Tibial liner
6663.50.214	CR #2 h. 14 mm	CR Mobile Tibial liner
6663.50.217	CR #2 h. 17 mm	CR Mobile Tibial liner
6663.50.220	CR #2 h. 20 mm	CR Mobile Tibial liner
6663.50.310	CR #3 h. 10 mm	CR Mobile Tibial liner
6663.50.312	CR #3 h. 12 mm	CR Mobile Tibial liner
6663.50.314	CR #3 h. 14 mm	CR Mobile Tibial liner
6663.50.317	CR #3 h. 17 mm	CR Mobile Tibial liner
6663.50.320	CR #3 h. 20 mm	CR Mobile Tibial liner
6663.50.410	CR #4 h. 10 mm	CR Mobile Tibial liner


6663.50.412	CR #4 h. 12 mm	CR Mobile Tibial liner
6663.50.414	CR #4 h. 14 mm	CR Mobile Tibial liner
6663.50.417	CR #4 h. 17 mm	CR Mobile Tibial liner
6663.50.420	CR #4 h. 20 mm	CR Mobile Tibial liner
6663.50.510	CR #5 h. 10 mm	CR Mobile Tibial liner
6663.50.512	CR #5 h. 12 mm	CR Mobile Tibial liner
6663.50.514	CR #5 h. 14 mm	CR Mobile Tibial liner
6663.50.517	CR #5 h. 17 mm	CR Mobile Tibial liner
6663.50.520	CR #5 h. 20 mm	CR Mobile Tibial liner
6662.50.010	UC #0 h. 10 mm	UC Mobile Tibial Liners
6662.50.012	UC #0 h. 12 mm	UC Mobile Tibial Liners
6662.50.014	UC #0 h. 14 mm	UC Mobile Tibial Liners
6662.50.017	UC #0 h. 17 mm	UC Mobile Tibial Liners
6662.50.020	UC #0 h. 20 mm	UC Mobile Tibial Liners
6662.50.110	UC #1 h. 10 mm	UC Mobile Tibial Liners
6662.50.112	UC #1 h. 12 mm	UC Mobile Tibial Liners
6662.50.114	UC #1h. 14 mm	UC Mobile Tibial Liners
6662.50.117	UC #1 h. 17 mm	UC Mobile Tibial Liners
6662.50.120	UC #1 h. 20 mm	UC Mobile Tibial Liners
6662.50.210	UC #2 h. 10 mm	UC Mobile Tibial Liners
6662.50.212	UC #2 h. 12 mm	UC Mobile Tibial Liners
6662.50.214	UC #2 h. 14 mm	UC Mobile Tibial Liners
6662.50.217	UC #2 h. 17 mm	UC Mobile Tibial Liners
6662.50.220	UC #2 h. 20 mm	UC Mobile Tibial Liners
6662.50.310	UC #3 h. 10 mm	UC Mobile Tibial Liners
6662.50.312	UC #3 h. 12 mm	UC Mobile Tibial Liners
6662.50.314	UC #3 h. 14 mm	UC Mobile Tibial Liners
6662.50.317	UC #3 h. 17 mm	UC Mobile Tibial Liners
6662.50.320	UC #3 h. 20 mm	UC Mobile Tibial Liners
6662.50.410	UC #4 h. 10 mm	UC Mobile Tibial Liners
6662.50.412	UC #4 h. 12 mm	UC Mobile Tibial Liners
6662.50.414	UC #4 h. 14 mm	UC Mobile Tibial Liners
6662.50.417	UC #4 h. 17 mm	UC Mobile Tibial Liners
6662.50.420	UC #4 h. 20 mm	UC Mobile Tibial Liners
6662.50.510	UC #5 h. 10 mm	UC Mobile Tibial Liners
6662.50.512	UC #5 h. 12 mm	UC Mobile Tibial Liners
6662.50.514	UC #5 h. 14 mm	UC Mobile Tibial Liners
6662.50.517	UC #5 h. 17 mm	UC Mobile Tibial Liners
6662.50.520	UC #5 h. 20 mm	UC Mobile Tibial Liners
6664.50.010	PS #0 h. 10 mm	PS Mobile Tibial Liners
6664.50.012	PS #0 h. 12 mm	PS Mobile Tibial Liners
6664.50.014	PS #0 h. 14 mm	PS Mobile Tibial Liners
6664.50.017	PS #0 h. 17 mm	PS Mobile Tibial Liners

6664.50.020	PS #0 h. 20 mm	PS Mobile Tibial Liners
6664.50.110	PS #1 h. 10 mm	PS Mobile Tibial Liners
6664.50.112	PS #1 h. 12 mm	PS Mobile Tibial Liners
6664.50.114	PS #1h. 14 mm	PS Mobile Tibial Liners
6664.50.117	PS #1 h. 17 mm	PS Mobile Tibial Liners
6664.50.120	PS #1 h. 20 mm	PS Mobile Tibial Liners
6664.50.210	PS #2 h. 10 mm	PS Mobile Tibial Liners
6664.50.212	PS #2 h. 12 mm	PS Mobile Tibial Liners
6664.50.214	PS #2 h. 14 mm	PS Mobile Tibial Liners
6664.50.217	PS #2 h. 17 mm	PS Mobile Tibial Liners
6664.50.220	PS #2 h. 20 mm	PS Mobile Tibial Liners
6664.50.310	PS #3 h. 10 mm	PS Mobile Tibial Liners
6664.50.312	PS #3 h. 12 mm	PS Mobile Tibial Liners
6664.50.314	PS #3 h. 14 mm	PS Mobile Tibial Liners
6664.50.317	PS #3 h. 17 mm	PS Mobile Tibial Liners
6664.50.320	PS #3 h. 20 mm	PS Mobile Tibial Liners
6664.50.410	PS #4 h. 10 mm	PS Mobile Tibial Liners
6664.50.412	PS #4 h. 12 mm	PS Mobile Tibial Liners
6664.50.414	PS #4 h. 14 mm	PS Mobile Tibial Liners
6664.50.417	PS #4 h. 17 mm	PS Mobile Tibial Liners
6664.50.420	PS #4 h. 20 mm	PS Mobile Tibial Liners
6664.50.510	PS #5 h. 10 mm	PS Mobile Tibial Liners
6664.50.512	PS #5 h. 12 mm	PS Mobile Tibial Liners
6664.50.514	PS #5 h. 14 mm	PS Mobile Tibial Liners
6664.50.517	PS #5 h. 17 mm	PS Mobile Tibial Liners
6664.50.520	PS #5 h. 20 mm	PS Mobile Tibial Liners

**SECTION 4 – EXAMPLE OF LABELS FOR MULTIGEN PLUS – CCK**

**Data Legend**

(the information which changes in the other labels of the same device is squared and showed in the table below).

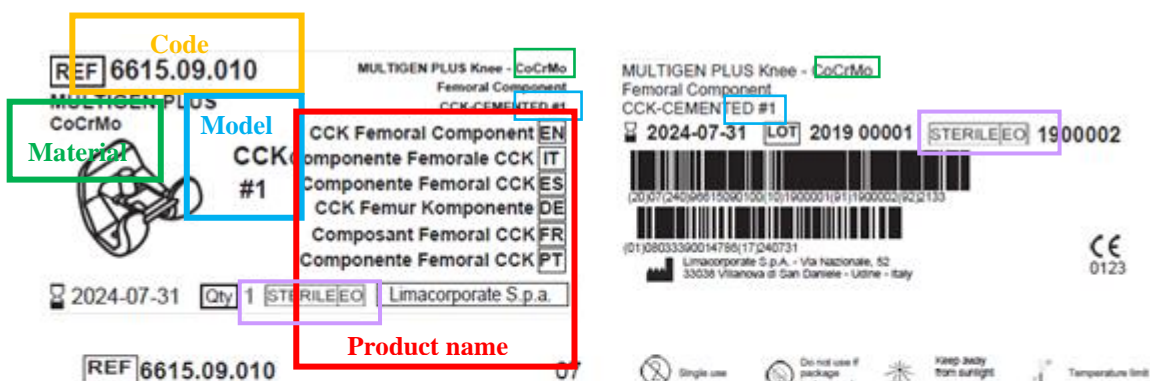



Code	Model	Material	Product name	Sterilization method
6615.09.010	CCK #1	CoCrMo	CCK- CEMENTED Femoral Components	EtO/Gamma
6615.09.020	CCK #2	CoCrMo	CCK- CEMENTED Femoral Components	EtO/Gamma
6615.09.030	CCK #3	CoCrMo	CCK- CEMENTED Femoral Components	EtO/Gamma
6615.09.040	CCK #4	CoCrMo	CCK- CEMENTED Femoral Components	EtO/Gamma
6615.09.050	CCK #5	CoCrMo	CCK- CEMENTED Femoral Components	EtO/Gamma
6645.50.110	CCK #1 h10	UHMWPE + Ti6Al4V	CCK Tibial Liner	EtO
6645.50.112	CCK #1 h12	UHMWPE + Ti6Al4V	CCK Tibial Liner	EtO
6645.50.114	CCK #1 h14	UHMWPE + Ti6Al4V	CCK Tibial Liner	EtO
6645.50.117	CCK #1 h17	UHMWPE + Ti6Al4V	CCK Tibial Liner	EtO
6645.50.120	CCK #1 h20	UHMWPE + Ti6Al4V	CCK Tibial Liner	EtO
6645.50.210	CCK #2 h10	UHMWPE + Ti6Al4V	CCK Tibial Liner	EtO
6645.50.212	CCK #2 h12	UHMWPE + Ti6Al4V	CCK Tibial Liner	EtO
6645.50.214	CCK #2 h14	UHMWPE + Ti6Al4V	CCK Tibial Liner	EtO
6645.50.217	CCK #2 h17	UHMWPE + Ti6Al4V	CCK Tibial Liner	EtO
6645.50.220	CCK #2 h20	UHMWPE + Ti6Al4V	CCK Tibial Liner	EtO
6645.50.310	CCK #3 h10	UHMWPE + Ti6Al4V	CCK Tibial Liner	EtO
6645.50.312	CCK #3 h12	UHMWPE + Ti6Al4V	CCK Tibial Liner	EtO
6645.50.314	CCK #3 h14	UHMWPE + Ti6Al4V	CCK Tibial Liner	EtO
6645.50.317	CCK #3 h17	UHMWPE + Ti6Al4V	CCK Tibial Liner	EtO

6645.50.320	CCK #3 h20	UHMWPE + Ti6Al4V	CCK Tibial Liner	EtO
6645.50.410	CCK #4 h10	UHMWPE + Ti6Al4V	CCK Tibial Liner	EtO
6645.50.412	CCK #4 h12	UHMWPE + Ti6Al4V	CCK Tibial Liner	EtO
6645.50.414	CCK #4 h14	UHMWPE + Ti6Al4V	CCK Tibial Liner	EtO
6645.50.417	CCK #4 h17	UHMWPE + Ti6Al4V	CCK Tibial Liner	EtO
6645.50.420	CCK #4 h20	UHMWPE + Ti6Al4V	CCK Tibial Liner	EtO
6645.50.510	CCK #5 h10	UHMWPE + Ti6Al4V	CCK Tibial Liner	EtO
6645.50.512	CCK #5 h12	UHMWPE + Ti6Al4V	CCK Tibial Liner	EtO
6645.50.514	CCK #5 h14	UHMWPE + Ti6Al4V	CCK Tibial Liner	EtO
6645.50.517	CCK #5 h17	UHMWPE + Ti6Al4V	CCK Tibial Liner	EtO
6645.50.520	CCK #5 h20	UHMWPE + Ti6Al4V	CCK Tibial Liner	EtO

**SECTION 5 – EXAMPLE OF LABELS FOR MULTIGEN PLUS – H**

**Data Legend**

(the information which changes in the other labels of the same device is squared and showed in the table below).



**Code** (yellow box): REF 6616.09.010

**Material** (green box): CoCrMo+CFR PEEK+Ti6Al4V

**Model** (blue box): H #1

**Product name** (red box): H Femoral Component

**Lot/Expiration** (purple box): 2024-07-31 | LOT 2019 00001 | STERILE EO | 900002

Other visible text on labels includes: MULTIGEN PLUS, Hinged Knee, Femoral Component H-CEMENTED #1, and manufacturer information: Limacorporate S.p.A., Via Nazionale, 52, 33036 Villanova di San Daniele - Udine - Italy.



Code	Model	Material	Product name	Sterilization method
6616.09.010	H #1	CoCrMo + CFR PEEK + Ti6Al4V	H CEMENTED Femoral Component	EtO/Gamma
6616.09.020	H #2	CoCrMo + CFR PEEK + Ti6Al4V	H CEMENTED Femoral Component	EtO/Gamma
6616.09.030	H #3	CoCrMo + CFR PEEK + Ti6Al4V	H CEMENTED Femoral Component	EtO/Gamma
6616.09.040	H #4	CoCrMo + CFR PEEK + Ti6Al4V	H CEMENTED Femoral Component	EtO/Gamma
6616.09.050	H #5	CoCrMo + CFR PEEK + Ti6Al4V	H CEMENTED Femoral Component	EtO/Gamma
6620.09.110	H #1	CoCrMo + CFR PEEK	H CEMENTED Tibial Plate	EtO/Gamma
6620.09.120	H #2	CoCrMo + CFR PEEK	H CEMENTED Tibial Plate	EtO/Gamma

6620.09.130	H #3	CoCrMo + CFR PEEK	H CEMENTED Tibial Plate	EtO/Gamma
6620.09.140	H #4	CoCrMo + CFR PEEK	H CEMENTED Tibial Plate	EtO/Gamma
6620.09.150	H #5	CoCrMo + CFR PEEK	H CEMENTED Tibial Plate	EtO/Gamma
6660.50.110	H #1 h 10	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.112	H #1 h 12	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.114	H #1 h 14	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.117	H #1 h 17	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.120	H #1 h 20	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.124	H #1 h 24	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.210	H #2 h 10	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.212	H #2 h 12	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.214	H #2 h 14	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.217	H #2 h 17	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.220	H #2 h 20	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.224	H #2 h 24	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.310	H #3 h 10	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.312	H #3 h 12	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.314	H #3 h 14	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.317	H #3 h 17	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.320	H #3 h 20	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.324	H #3 h 24	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.410	H #4 h 10	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.412	H #4 h 12	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.414	H #4 h 14	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.417	H #4 h 17	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.420	H #4 h 20	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.424	H #4 h 24	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.510	H #5 h 10	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO




6660.50.512	H #5 h 12	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.514	H #5 h 14	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.517	H #5 h 17	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.520	H #5 h 20	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO
6660.50.524	H #5 h 24	UHMWPE + CoCrMo + Ti6Al4V	H Tibial Liner + Hinge	EtO

**SECTION 6 – EXAMPLE OF LABELS FOR AUGMENTS (Ti6Al4V)**

- **Tibial augments**

**Data Legend**

(the information which changes in the other labels of the same device is squared and showed in the table below).

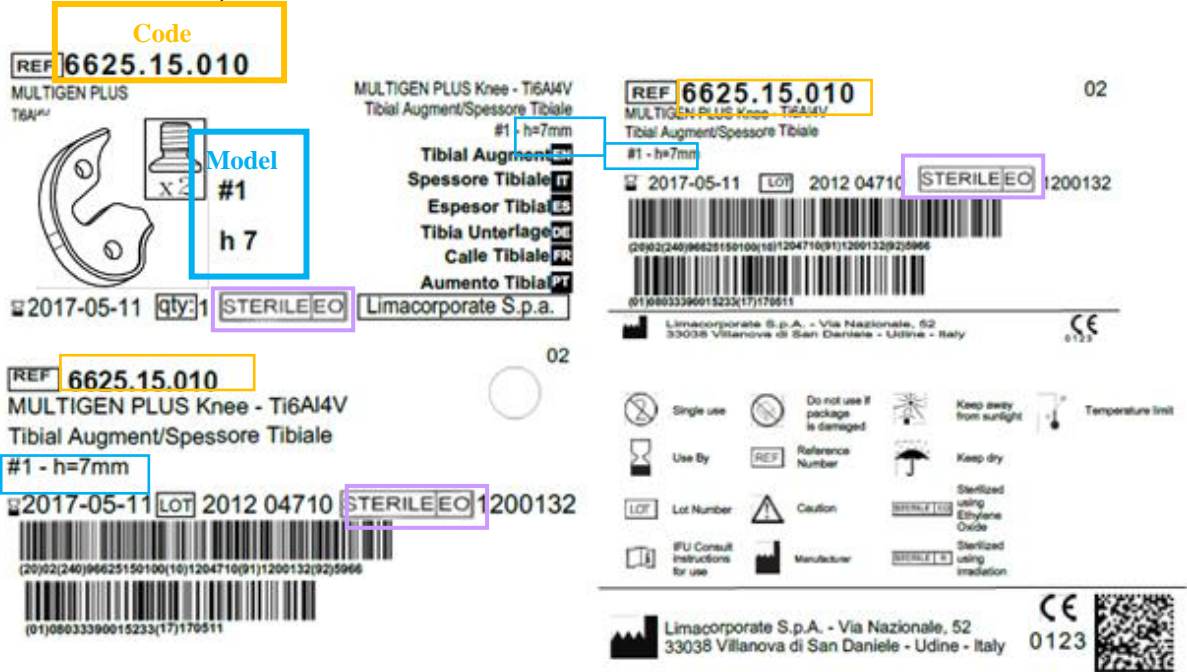


Code	Model	Sterilization method
6625.15.010	#1 h 7	EtO/Radiation
6625.15.020	#1 h 12	EtO/Radiation
6626.15.010	#2 h 7	EtO/Radiation
6626.15.020	#2 h 12	EtO/Radiation
6628.15.010	#3 h 7	EtO/Radiation
6628.15.020	#3 h 12	EtO/Radiation
6630.15.010	#4 h 7	EtO/Radiation
6630.15.020	#4 h 12	EtO/Radiation
6632.15.010	#5 h 7	EtO/Radiation
6632.15.020	#5 h 12	EtO/Radiation

- **H – Tibial augments**

**Data Legend**

(the information which changes in the other labels of the same device is squared and showed in the table below).

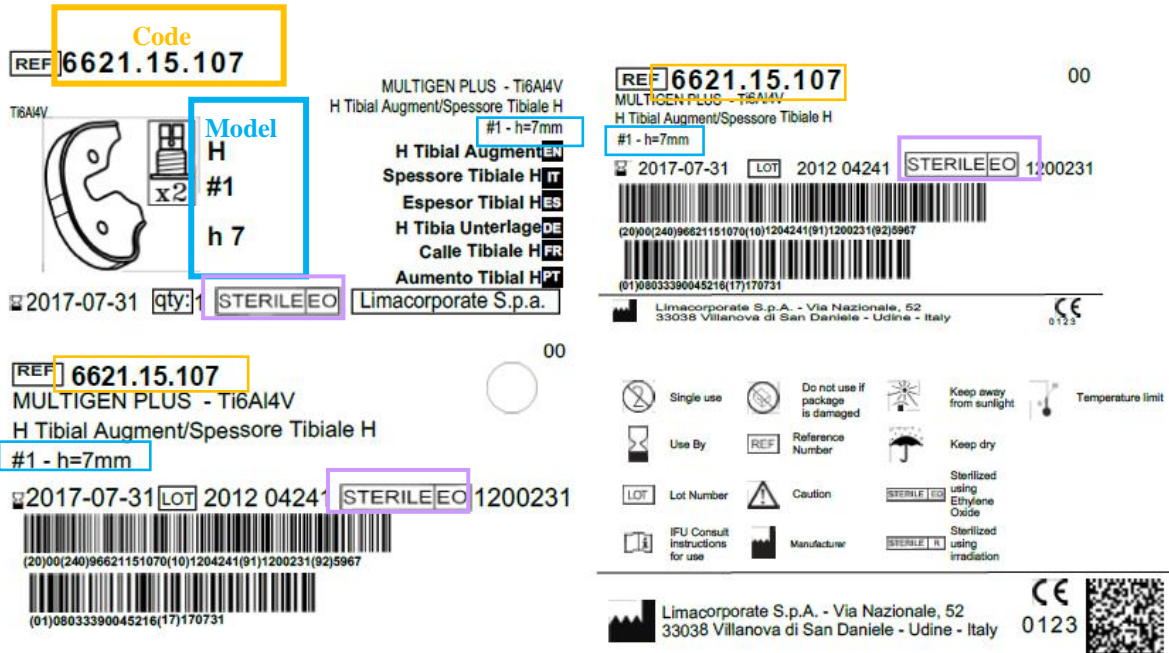

**Code**  
REF 6621.15.107

MULTIGEN PLUS - T16A14V  
H Tibial Augment/Spessore Tibiale H  
#1 - h=7mm

**Model**  
H  
#1  
h 7

H Tibial Augment  
Spessore Tibiale  
Espesor Tibial  
H Tibia Unterlage  
Calle Tibiale  
Aumento Tibial

2017-07-31 qty:1 STERILE EO Limacorporate S.p.a.

00

REF 6621.15.107  
MULTIGEN PLUS - T16A14V  
H Tibial Augment/Spessore Tibiale H  
#1 - h=7mm

2017-07-31 LOT 2012 04241 STERILE EO 1200231

(20)00(240)96621151070(10)1204241(91)1200231(92)5967  
(01)08033390045216(17)170731

Limacorporate S.p.A. - Via Nazionale, 52  
33038 Villanova di San Daniele - Udine - Italy

CE 0123

Single use  
Do not use if package is damaged  
Keep away from sunlight  
Temperature limit  
Use By  
Reference Number  
Keep dry  
Lot Number  
Caution  
Sterilized using Ethylene Oxide  
IFU Consult instructions for use  
Manufacturer  
Sterilized using irradiation

Limacorporate S.p.A. - Via Nazionale, 52  
33038 Villanova di San Daniele - Udine - Italy

CE 0123

Code	Model	Sterilization method
6621.15.107	H #1 h 7	EtO/Radiation
6621.15.112	H#1 h 12	EtO/Radiation
6621.15.207	H #2 h 7	EtO/Radiation
6621.15.212	H #2 h 12	EtO/Radiation
6621.15.307	H #3 h 7	EtO/Radiation
6621.15.312	H #3 h 12	EtO/Radiation
6621.15.407	H #4 h 7	EtO/Radiation
6621.15.412	H #4 h 12	EtO/Radiation
6621.15.507	H #5 h 7	EtO/Radiation
6621.15.512	H #5 h 12	EtO/Radiation

• **Femoral augments**


**Data Legend**

(the information which changes in the other labels of the same device is squared and showed in the table below).

**Distal**

**Code**  
REF 6671.15.105

MULTIGEN PLUS  
Ti6AlV



**#1**  
**h 5**  
**Model**

MULTIGEN PLUS Knee - Ti6AlV  
Femoral Augment/Spessore Femorale  
#1-5mm Distal  
Femoral Augment **EN**  
Spessore Femorale **IT**  
Espesor Femoral **ES**  
Femur Unterlage **DE**  
Calle Femoral **FR**  
Aumento Femoral **PT**

2017-02-07 qty:1 **STERILE EO** Limacorporate S.p.a.

REF 6671.15.105 01

MULTIGEN PLUS Knee - Ti6AlV  
Femoral Augment/Spessore Femorale  
#1-5mm Distal

2017-02-07 **LOT** 2011 04403 **STERILE EO** 1200024




(20)01(240)96671151050(10)1104403(9)11200024(9)25968  
(01)09033990017114(17)170207

Limacorporate S.p.A. - Via Nazionale, 52  
33038 Villanova di San Daniele - Udine - Italy **CE**

REF 6671.15.105 01

MULTIGEN PLUS Knee - Ti6AlV  
Femoral Augment/Spessore Femorale  
#1-5mm Distal

2017-02-07 **LOT** 2011 04403 **STERILE EO** 1200024



(20)01(240)96671151050(10)1104403(9)11200024(9)25968  
(01)09033990017114(17)170207

Single use Do not use if package is damaged Keep away from sunlight Temperature limit

Use By REF Reference Number Keep dry

**LOT** Lot Number **CAUTION** Caution Sterilized using Ethylene Oxide

IFU Consult instructions for use Manufacturer Sterilized using irradiation


Limacorporate S.p.A. - Via Nazionale, 52  
33038 Villanova di San Daniele - Udine - Italy **CE** 0123



**Posterior**

**Code**  
REF 6672.15.105

MULTIGEN PLUS  
Ti6AlV



**#1**  
**h 5**  
**Model**

MULTIGEN PLUS Knee - Ti6AlV  
Femoral Augment/Spessore Femorale  
#1-5mm Posterior  
Femoral Augment **EN**  
Spessore Femorale **IT**  
Espesor Femoral **ES**  
Femur Unterlage **DE**  
Calle Femoral **FR**  
Aumento Femoral **PT**

2020-02-28 qty:1 **STERILE EO** Limacorporate S.p.a.

REF 6672.15.105 01

MULTIGEN PLUS Knee - Ti6AlV  
Femoral Augment/Spessore Femorale  
#1-5mm Posterior

2020-02-28 **LOT** 2014 14918 **STERILE EO** 500054



(20)01(240)96672151050(10)1414918(9)11500054(9)25969  
(01)09033990017213(17)200228

Limacorporate S.p.A. - Via Nazionale, 52  
33038 Villanova di San Daniele - Udine - Italy **CE**

REF 6672.15.105 01

MULTIGEN PLUS Knee - Ti6AlV  
Femoral Augment/Spessore Femorale  
#1-5mm Posterior

2020-02-28 **LOT** 2014 14918 **STERILE EO** 1500054



(20)01(240)96672151050(10)1414918(9)11500054(9)25969  
(01)09033990017213(17)200228


Single use Do not use if package is damaged Keep away from sunlight Temperature limit

Use By REF Reference Number Keep dry

**LOT** Lot Number **CAUTION** Caution Sterilized using Ethylene Oxide

IFU Consult instructions for use Manufacturer Sterilized using irradiation

Limacorporate S.p.A. - Via Nazionale, 52  
33038 Villanova di San Daniele - Udine - Italy **CE** 0123



<b>Code</b>	<b>Model</b>	<b>Sterilization method</b>
6671.15.105	# 1 h 5	EtO/Radiation
6671.15.205	#2 h 5	EtO/Radiation
6671.15.210	#2 h 10	EtO/Radiation
6671.15.305	#3 h 5	EtO/Radiation
6671.15.310	#3 h 10	EtO/Radiation
6671.15.405	#4 h 5	EtO/Radiation
6671.15.410	#4 h 10	EtO/Radiation
6671.15.505	#5 h 5	EtO/Radiation
6671.15.510	#5 h 10	EtO/Radiation
6672.15.105	# 1 h 5	EtO/Radiation
6672.15.205	#2 h 5	EtO/Radiation
6672.15.210	#2 h 10	EtO/Radiation
6672.15.305	#3 h 5	EtO/Radiation
6672.15.310	#3 h 10	EtO/Radiation
6672.15.405	#4 h 5	EtO/Radiation
6672.15.410	#4 h 10	EtO/Radiation
6672.15.505	#5 h 5	EtO/Radiation
6672.15.510	#5 h 10	EtO/Radiation

**SECTION 7 – EXAMPLE OF LABELS FOR STEMS (Ti6Al4V) AND MODULES (Ti6Al4V)**

- **Tibial Stems**

**Data Legend**

(the information which changes in the other labels of the same device is squared and showed in the table below).

<p><b>Code</b> REF 6665.15.020</p> <p><b>Model</b> h60</p>	<p><b>Product name</b> Tibial Stem/Stelo Tibiale</p>	
<p><b>Product name</b> Tibial Stem/Stelo Tibiale</p>		

- **CCK/H Stems**


<p><b>Code</b> REF 6647.15.140</p> <p><b>Model</b> Dia. 14mm</p>	<p><b>Product name</b> CCK/H Stems</p>	
<p><b>Product name</b> CCK/H Stems</p>		

Code	Model	Product name
------	-------	--------------

6665.15.020	h 60	Tibial Stem
6665.15.040	h 90	Tibial Stem
6647.15.140	Dia 14 mm, length 60	CCK/H Stem
6647.15.160	Dia 16 mm, length 60	CCK/H Stem
6647.15.180	Dia 18 mm, length 85	CCK/H Stem
6647.15.200	Dia 20 mm, length 85	CCK/H Stem
6647.15.220	Dia 22 mm, length 110	CCK/H Stem
6647.15.240	Dia 24 mm, length 110	CCK/H Stem

• **CCH-Modules**

**Code**  
REF 6647.15.310  
MULTIGEN PLUS Ti6Al4V



**CCK #S Model**


MULTIGEN PLUS Knee - Ti6Al4V  
CCK Tibial Module / Modulo Tibiale  
Straight / Dritto SHORT

CCK Straight Tibia Mod #S EN  
CCK Modulo Tib. Dritto #S IT  
CCK Mod Tibial Recto #S ES  
CCK Senkr Tibiamodul #S DE  
CCK Conn. Tibial Droit #S FR  
CCK Mod Tibial Recto #S PT

2017-03-27 qty:1 STERILE EO Limacorporate S.p.a.

REF 6647.15.310 01  
MULTIGEN PLUS Knee - Ti6Al4V  
CCK Tibial Module / Modulo Tibiale  
Straight / Dritto SHORT

2017-03-27 LOT 2011 12980 STERILE EO 1200078




(20)01(240)96647153100(10)1112980(91)1200078(92)5972  
(01)08033390041539(17)170327

Limacorporate S.p.A. - Via Nazionale, 52  
33038 Villanova di San Daniele - Udine - Italy

REF 6647.15.310  
MULTIGEN PLUS Knee - Ti6Al4V  
CCK Tibial Module / Modulo Tibiale  
Straight / Dritto SHORT

**Product name**

2017-03-27 LOT 2011 12980 STERILE EO 1200078



(20)01(240)96647153100(10)1112980(91)1200078(92)5972  
(01)08033390041539(17)170327

01

Single use Do not use if package is damaged Keep away from sunlight Temperature limit


Use By REF Reference Number Keep dry

LOT Lot Number Caution STERILE EO Sterilized using Ethylene Oxide

IFU Consult instructions for use Manufacturer STERILE IR Sterilized using irradiation


Limacorporate S.p.A. - Via Nazionale, 52  
33038 Villanova di San Daniele - Udine - Italy

CE 0123



• **CCK/H Femoral Modules**

**Code**  
REF 6647.15.410  
MULTIGEN PLUS Ti6Al4V




**#S R-L Model**

MULTIGEN PLUS Knee - Ti6Al4V  
Femoral Module CCK/H  
SHORT R-L

Femoral Module #S R-L EN  
Modulo Femorale #S D-S IT  
Modulo Femoral #S D-ES  
Femuralmodul #S R-L DE

REF 6647.15.410 01  
MULTIGEN PLUS Knee - Ti6Al4V  
Femoral Module CCK/H  
SHORT R-L


2024-07-31 LOT 2019 00001 STERILE EO 19 00002



**H tibial Modules**

**Data Legend**

(the information which changes in the other labels of the same device is squared and showed in the table below).

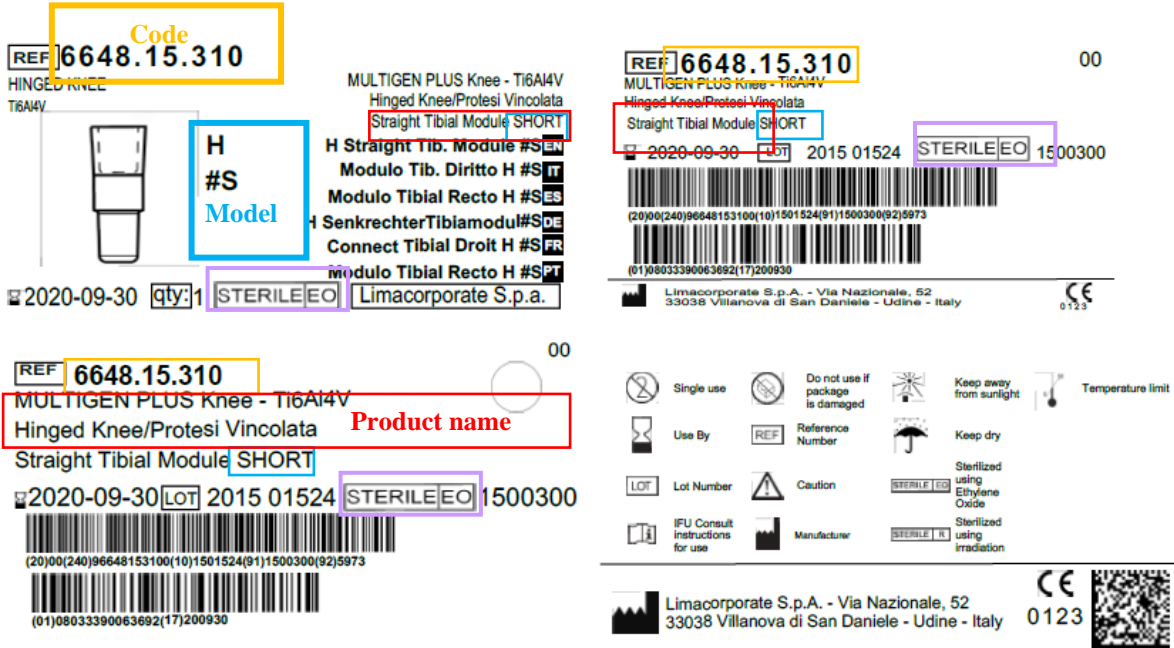

Code	Model	Product name	Sterilization method
6647.15.310	Straight SHORT	CCK Tibial Module	EtO/Radiation
6647.15.320	SHORT Offset +3 mm	CCK Tibial Module	EtO/Radiation
6647.15.330	SHORT Offset +6 mm	CCK Tibial Module	EtO/Radiation
6647.15.340	Straight LONG	CCK Tibial Module	EtO/Radiation
6647.15.350	LONG Offset +3 mm	CCK Tibial Module	EtO/Radiation
6647.15.360	LONG Offset +6 mm	CCK Tibial Module	EtO/Radiation
6647.15.410	SHORT R – L	CCK/H Femoral Module	EtO/Radiation
6647.15.420	SHORT R+3mm - L-3mm	CCK/H Femoral Module	EtO/Radiation
6647.15.430	SHORT R-3mm - L+3mm	CCK/H Femoral Module	EtO/Radiation
6647.15.440	LONG R – L	CCK/H Femoral Module	EtO/Radiation
6647.15.450	LONG R+3mm - L-3mm	CCK/H Femoral Module	EtO/Radiation
6647.15.460	LONG R-3mm - L+3mm	CCK/H Femoral Module	EtO/Radiation
6648.15.310	H Straight SHORT	H Tibial Module	EtO/Radiation
6648.15.320	H SHORT Offset +3 mm	H Tibial Module	EtO/Radiation
6648.15.330	H SHORT Offset +6 mm	H Tibial Module	EtO/Radiation
6648.15.340	H Straight LONG	H Tibial Module	EtO/Radiation
6648.15.350	H LONG Offset +3 mm	H Tibial Module	EtO/Radiation
6648.15.360	H LONG Offset +6 mm	H Tibial Module	EtO/Radiation

**SECTION 8 – EXAMPLE OF LABELS FOR PATELLAR PROSTHESIS**




**Data Legend**

(the information which changes in the other labels of the same device is squared and showed in the table below).

**Code**  
REF **6695.50.103**

MULTIGEN PLUS  
UHMWPE



**Dia 28**  
**h8**

**Model**

2022-06-30 qty: 1 **STERILE EO** Limacorporate S.p.a.


MULTIGEN PLUS Knee - UHMWPE  
Patellar Prosthesis/Protesi Rotulea  
Dia 28mm - h=8mm

Patellar Prosthesis **EN**  
Protesi Rotulea **IT**  
Rotula Protetica **ES**  
Patella Prothese **DE**  
Prothese de Rotule **FR**  
Rotula Protetica **PT**


REF **6695.50.103** 02

MULTIGEN PLUS Knee - UHMWPE  
Patellar Prosthesis/Protesi Rotulea  
Dia 28mm - h=8mm

2022-06-30 **LOT** 2016 AT184 **STERILE EO** 1700207



(20)02(240)96695501030(10)16AT184(91)1700207(92)7408



(01)08033390017350(17)220630

Limacorporate S.p.A. - Via Nazionale, 52  
33038 Villanova di San Daniele - Udine - Italy


**CE**  
0123


REF **6695.50.103**

MULTIGEN PLUS Knee - UHMWPE  
Patellar Prosthesis/Protesi Rotulea  
Dia 28mm - h=8mm

2022-06-30 **LOT** 2016 AT184 **STERILE EO** 1700207





(20)02(240)96695501030(10)16AT184(91)1700207(92)7408





(01)08033390017350(17)220630


02





 Single use


 Do not use if package is damaged


 Keep away from sunlight


 Temperature limit


 Use By


 Reference Number


 Keep dry


 Lot Number

 Caution

 Sterilized using Ethylene Oxide


 IFU Consult instructions for use

 Manufacturer

 Sterilized using irradiation

Limacorporate S.p.A. - Via Nazionale, 52  
33038 Villanova di San Daniele - Udine - Italy

**CE**  
0123



Code	Model
6695.50.103	Dia 28 h8
6695.50.105	Dia 32 h8
6695.50.005	Dia 32
6695.50.010	Dia 35
6695.50.020	Dia 38
6695.50.030	Dia 41