

# pCONUS 2 HPC

## Bifurcation Aneurysm Implant


Bifurcation Aneurysm Implant - Implantat für Bifurkationsaneurysmen - Implant pour anévrisme de bifurcation - Implanto dell'aneurisma della biforcazione - Implante para aneurisma con bifurcación - Implante bifurcado para tratamiento de aneurisma - Имплантат для лечения аневризмы бифуркации

**PCON2-HPC-4-15-6**

phenox GmbH  
Lise-Meitner-Allee 31 - 44801 Bochum, Germany  
Tel: +49 (0) 234 / 36919-0 - Fax: +49 (0) 234 / 36919-19  
www.phenox.net

**4 mm x 15 mm x 6 mm** ID **0.021"** **2.5 - 3.7 mm**  
Shaft Ø Shaft Length Crown Diameter Min. Microcatheter Vessel Ø

### HPC - Hydrophilic Polymer Coating

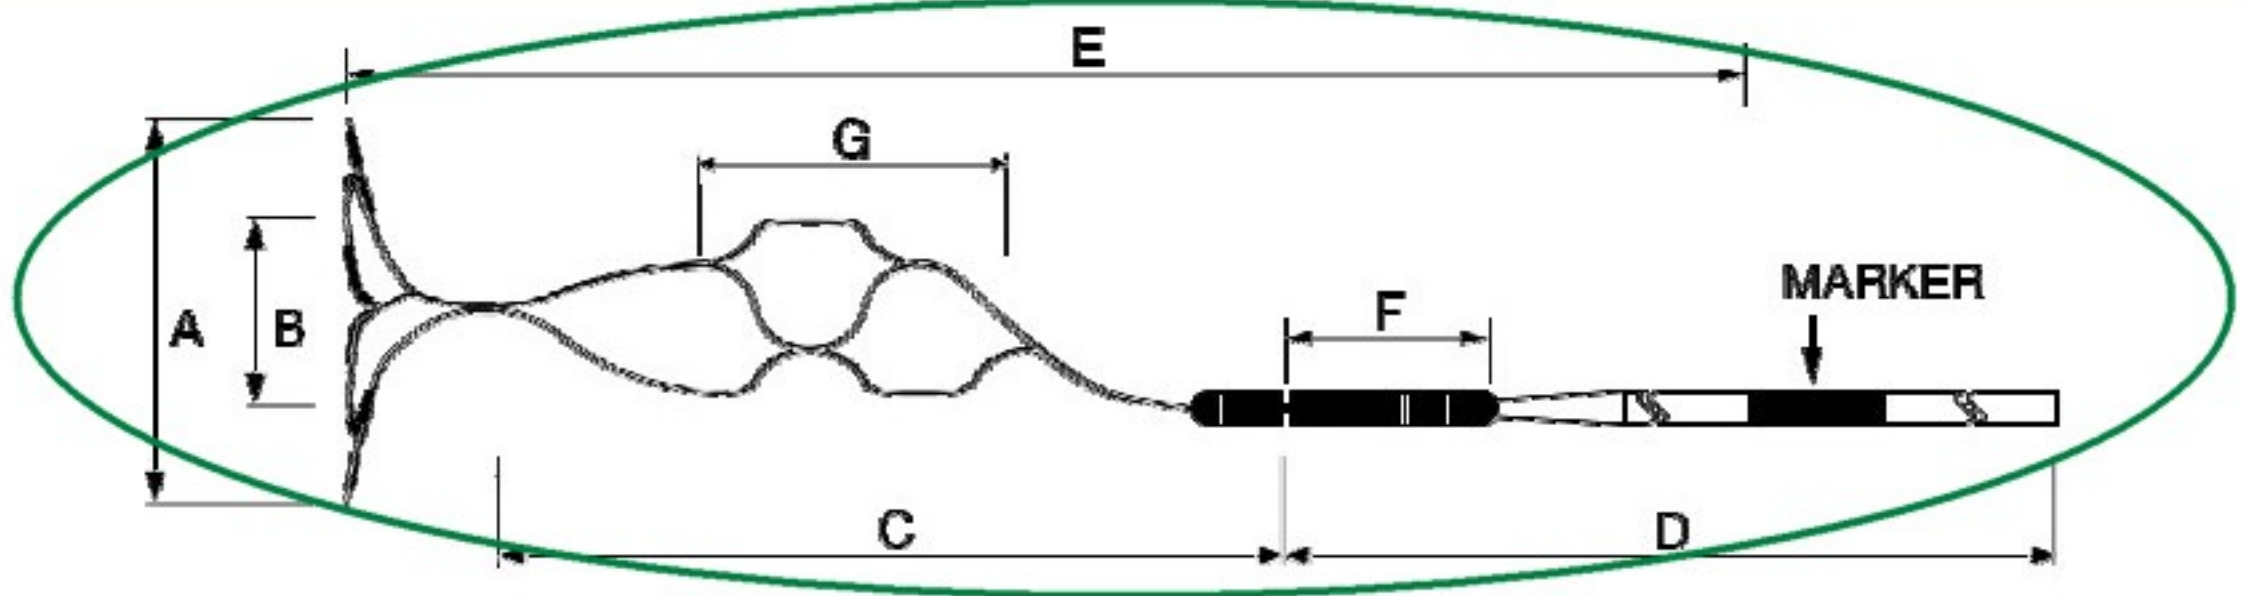

A: Crown Diameter [mm]	B: Shaft Diameter [mm]	C: Shaft Length [mm]	D: Insertion Wire Length [mm]	E: System Length [mm]	F: Marker Length [mm]	G: Working Length [mm]	Microcatheter Compatibility [Inch]	Vessel Diameter [mm]
6	4	15	1830	1275	30	7	Min. ID 0.021"	2.5 - 3.7

REF **PCON2-HPC-4-15-6** LOT 123456 2021-07 CONT 1 x pCONUS 2 HPC

pCONUS 2 HPC REF **PCON2-HPC-4-15-6** LOT 123456



(01)04260123782320(17)210630(10)123456

pCONUS 2 HPC REF **PCON2-HPC-4-15-6** LOT 123456



(01)04260123782320(17)210630(10)123456

pCONUS 2 HPC REF **PCON2-HPC-4-15-6** LOT 123456



(01)04260123782320(17)210630(10)123456

CE 0297

MAT NITi

STERILE EO  
Sterilized with Ethylene Oxide Gas

Consult instructions for use

Caution

Do not reuse

Keep dry

Keep away from sunlight

Do not use if the package is damaged

Do not resterilize

Non-sterile

LAB-B851-PCONUS2-HPC A - 2018/07

pCONUS 2 HPC Bifurcation Aneurysm Implant

4 mm x 15 mm x 6 mm



REF **PCON2-HPC-4-15-6**

LOT 123456 2021-07