

# Fox Plus: Box- and pouch-label new (OUS)

**Fox Plus** PTA Catheter (01)0000000000000(17)010131(10)000000(91)3000

REF LV\_ITNR LOT \*VOID LV\_EXPD

Ø BALLOON **3.0 mm** ↔ BALLOON **20 mm** ↔ USAB CAT **80 cm** SHEATH **5 Fr 1.67mm**

## Fox Plus


PTA Catheter

CONTENTS 1 Fox Plus OTW PTA Catheter

REF LV\_ITNR

LOT \*VOID

LV\_EXPD

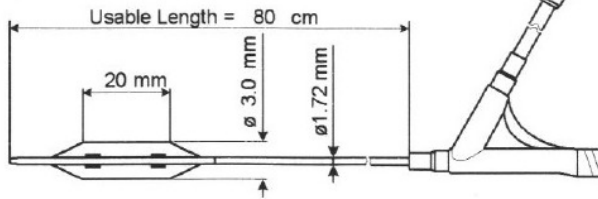

Ø BALLOON

**3.0 mm**

↔ BALLOON

**20 mm**

RBP

**18 bar**  
**1800 kPa**

↔ USAB CAT

**80 cm**

SHEATH

**5 Fr**  
**1.67 mm**

REC GW

**0.035"**  
**0.89 mm**



STERILE R

NON PYROGENIC



DIST



Abbott Vascular Devices Holland B.V.,  
Maastricht Airport, Bamfordweg 1,  
NL-6235 NS Ulestraten, The Netherlands  
Phone: +31 43 358 6751  
FAX: +31 43 358 6759

Abbott Laboratories Vascular Enterprises Ltd.,  
Dublin, Beringen Branch, Anthoptstrasse  
CH-8222 Beringen, Switzerland,  
Phone: +41 52 674 8550  
FAX: +41 52 674 8540

**Abbott**

© 2008 Abbott Laboratories

LA 007532001 005

DO NOT EXCEED!

RBP

\*\*

NPR

Balloon Compliance			Ø 3.0
	Pressure		Diameter
	[kPa]	[bar]	
	400	4	2.6
	500	5	2.7
	600	6	2.8
	700	7	2.8
	800	8	2.9
	900	9	3.0
*	1000	10	3.0
	1100	11	3.0
	1200	12	3.1
	1300	13	3.1
	1400	14	3.2
	1500	15	3.2
	1600	16	3.2
	1700	17	3.3
**	1800	18	3.3
	1900	19	3.3
	2000	20	3.4
	2100	21	3.4
	2200	22	3.4
	2300	23	-
*	2400	24	-

**Fox Plus** PTA Catheter (01)0000000000000(17)010131(10)000000(91)3000

Ø 3.0 mm ↔ 20 mm

**Fox Plus** PTA Catheter (01)0000000000000(17)010131(10)000000(91)3000


Ø 3.0 mm ↔ 20 mm

REF LV\_ITNR LOT \*VOID ↔ BALLOON 20 mm

**Fox Plus** PTA Catheter 3.0 mm ↔ BALLOON 20 mm

ALIVE Ltd., Dublin, Beringen Branch, CH-8222 Beringen, Phone: +41 52 674 8550 FAX: +41 52 674 8540

# Fox Plus: Compliance chart new (OUS/US)

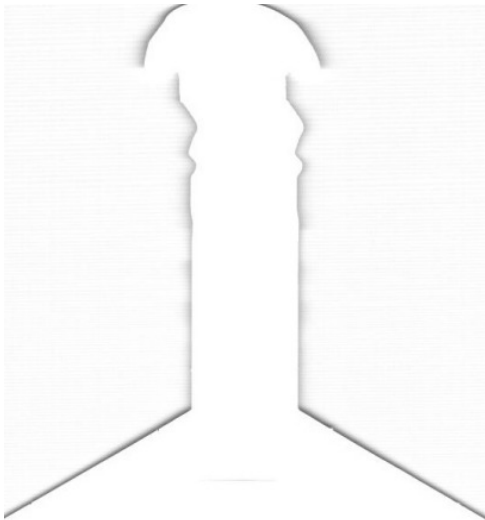

<b>Fox Plus PTA Catheter</b>				
<b>Balloon Compliance</b> $\phi$ 3.0				
	Pressure			Diameter
	[kPa]	[bar]	[atm]	[mm]
	400	4	4	2.6
	500	5	5	2.7
	600	6	6	2.8
	700	7	7	2.8
	800	8	8	2.9
	900	9	9	3.0
*	1000	10	10	3.0
	1100	11	11	3.0
	1200	12	12	3.1
	1300	13	13	3.1
	1400	14	14	3.2
	1500	15	15	3.2
	1600	16	16	3.2
	1700	17	17	3.3
**	1800	18	18	3.3
	1900	19	19	3.3
	2000	20	20	3.4
	2100	21	21	3.4
	2200	22	22	3.4
	2300	23	23	-
	2400	24	24	-
<div style="display: flex; justify-content: space-between; align-items: center;"> <span>LOT</span> <span>*VOID</span> </div>				

\*Nominal Pressure \*\*RBP Do not exceed

LA 007533001 003

DO NOT EXCEED


RBP

\*\*

NPR

\*

## Fox Plus: Box new

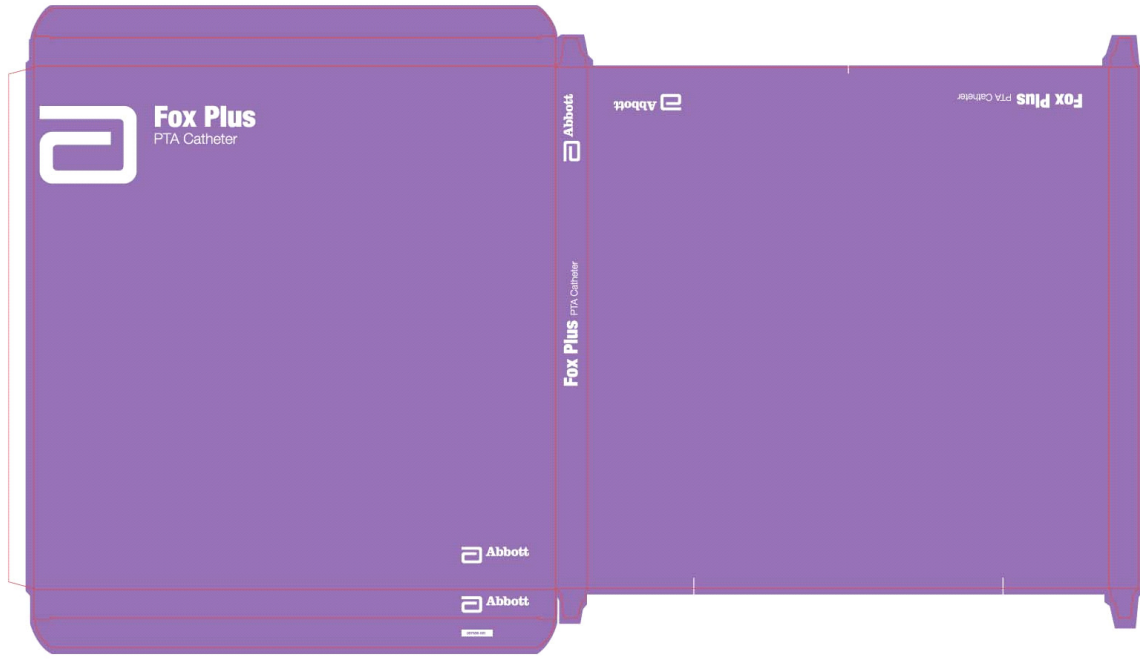

## Fox Plus: Blister new

Embossed Abbottlogo on blister adjusted as follows:

